

Start up Guide

LA and LT

Balance Series

1. CONTENT

Models: LA-225.C



Balance
x 1




Weighing pan
x 1




Draft shield
x 1



Centring ring
x 1



Bottom insert
x 1



Power adapter
x 1

Models: LA-164.C | LA-224.C | LA-314.C | LA-64 | LA-164 | LA-224 | LA-314 | LA-224.N | LA-314.N




Balance
x 1




Weighing pan
x 1



Draft shield
x 1



Bottom insert
x 1



Power adapter
x 1


Models: LT-363.C | LT-603.C | LT-363 | LT-603 | LT-363.N | LT-1003.N



Balance
x 1



Weighing pan
x 1




Draft shield
x 1



Grounding foot
x 1



Foot
x 3



Power adapter
x 1

Models: LT-1202.C | LT-2102.C | LT-4502.C | LT-1202 | LT-2102 | LT-4502 | LT-2102.N | LT-4502.N



Balance
x 1




Weighing pan
x 1



Grounding foot
x 1



Foot
x 3



Power adapter
x 1

Models: LT-6002.C | LT-6002



Balance
x 1



Weighing pan
x 1




Draft shield
x 1



Grounding foot
x 1




Foot
x 1




Power adapter
x 1

2. WORKROOM AND BASIC OPERATION GUIDELINES

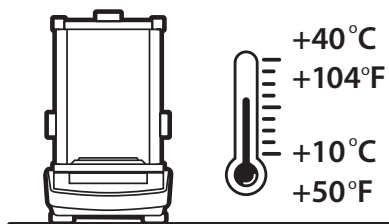


Operate the device in a room where the temperature ranges between 10–40 °C (50–104 °F) and where the relative humidity is below 80%.


Place the balance on a solid surface to ensure stability. To obtain stable and repeatable weighing results, an anti-vibration table is recommended.

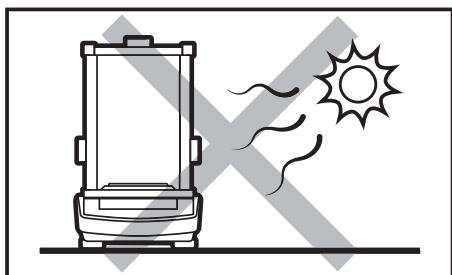


Place the balance away from heat sources. Avoid exposing the balance to the sunlight.

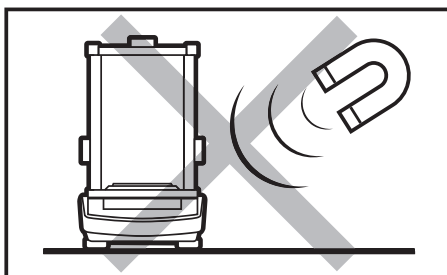


Avoid exposing the balance to a magnetic field. Do not weigh magnetic substances.

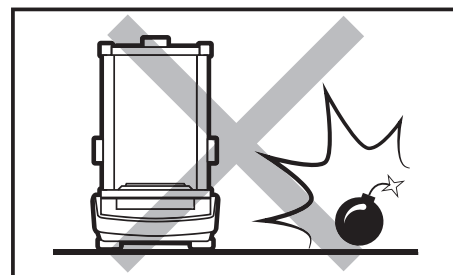


Do not place the balance in a hazardous area. Do not weigh explosive materials.

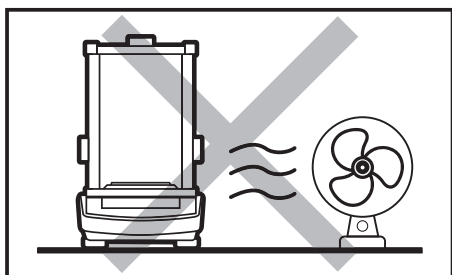

Avoid air drafts and air movements at the workstation.



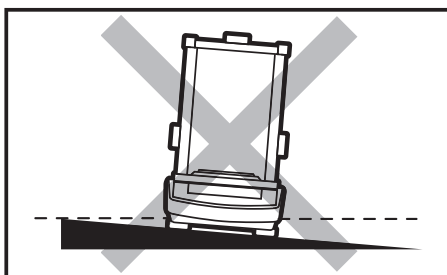


Make sure that the balance is placed on an even surface.

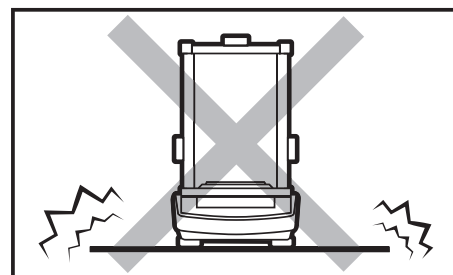

Do not place the balance on an unstable ground exposed to shocks and vibrations.

3. UNPACKING

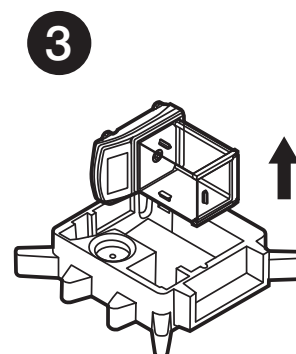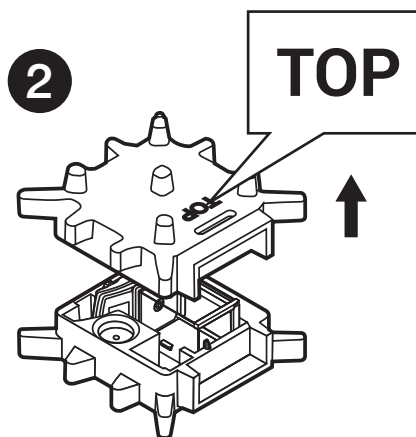
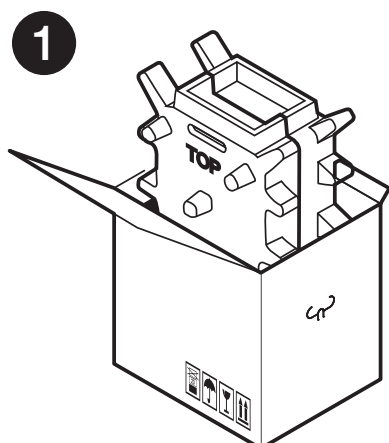


Keep the packaging should a warranty claim or service be required.

4. ACTIVITIES TO BE DONE PRIOR TO OPERATION



4.1. Remove transport lock

Models: LA-225.C | LA-164.C | LA-224.C | LA-314.C | LA-64 | LA-164 | LA-224 | LA-314 | LA-224.N | LA-314.N

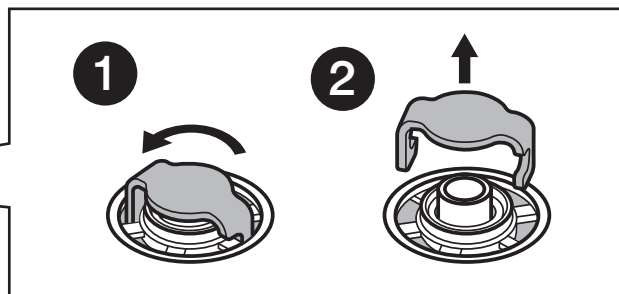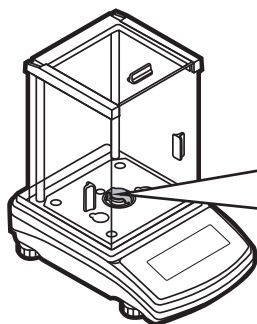

Keep the transport lock should a warranty claim or service be required.



Models: LT-363.C | LT-603.C | LT-1202.C | LT-2102.C | LT-4502.C | LT-6002.C | LT-363 | LT-603 | LT-2102 | LT-4502 | LT-6002 | LT-2102.N | LT-4502.N

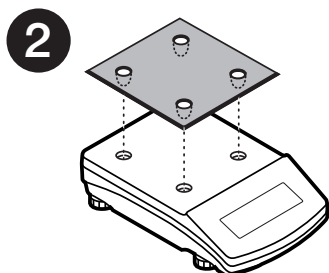

Keep the transport lock should a warranty claim or service be required.

4.2. Grounding spring check

Models: LA-225.C | LA-164.C | LA-224.C | LA-314.C | LA-64 | LA-164 | LA-224 | LA-314 | LA-224.N | LA-314.N

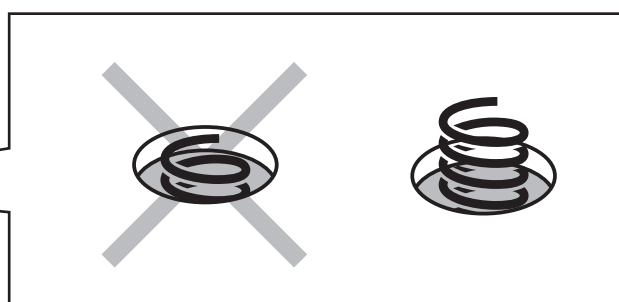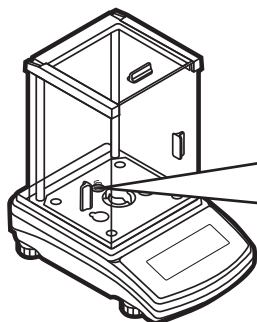


Check the grounding spring. Make sure that the grounding spring juts slightly out of the hole.

Models: LT-363.C | LT-603.C | LT-1202.C | LT-2102.C | LT-4502.C | LT-6002.C | LT-363 | LT-603 | LT-2102 | LT-4502 | LT-6002 | LT-2102.N | LT-4502.N




Grounding foot

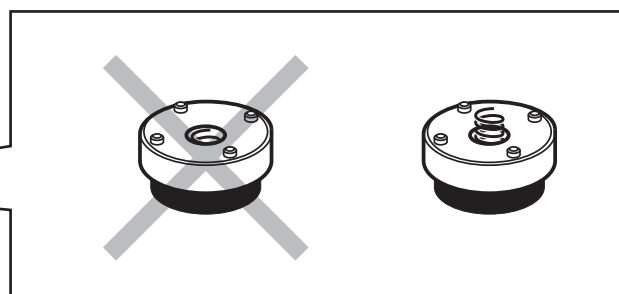


Check the grounding spring. Make sure that the grounding spring juts slightly out of the hole.

5. COMPONENTS ASSEMBLY


Models: LA-225.C

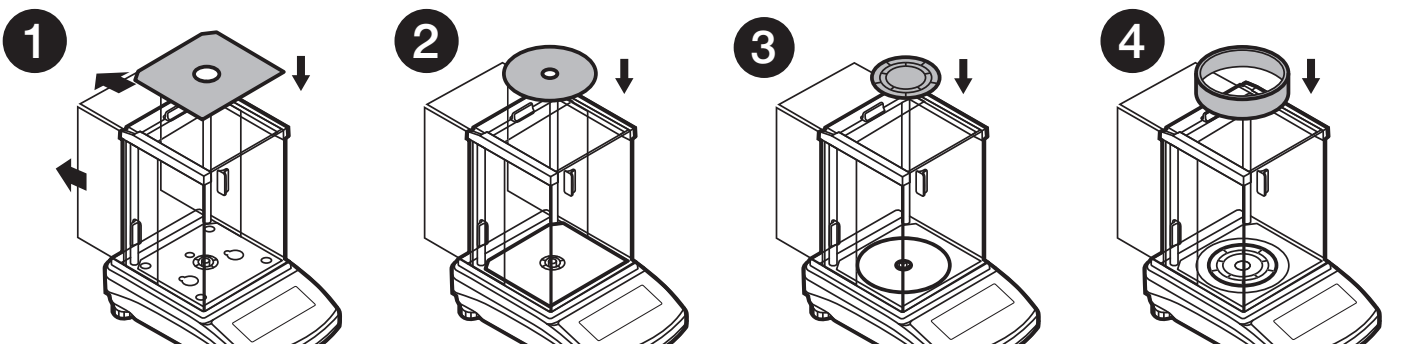


Models: LA-164.C | LA-224.C | LA-314.C | LA-64 | LA-164 | LA-224 | LA-314 | LA-224.N | LA-314.N

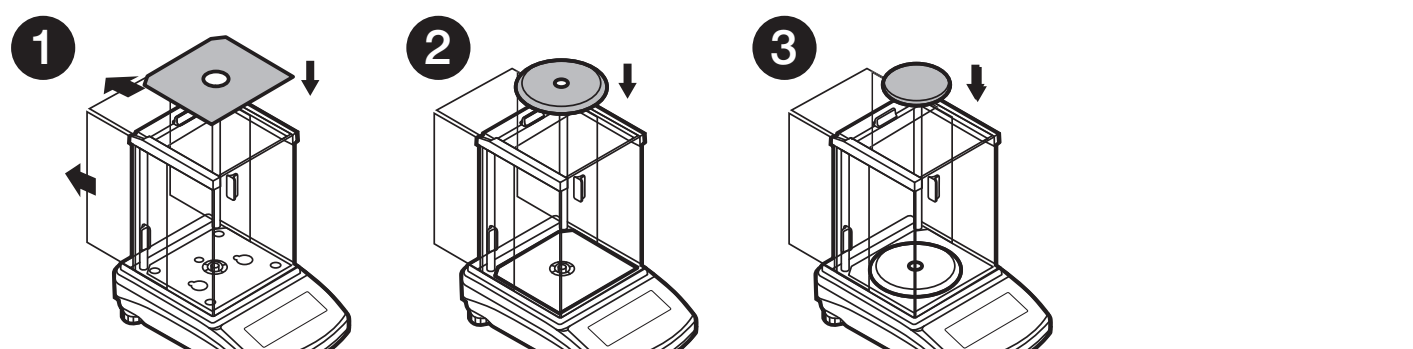


Models: LT-363.C | LT-603.C | LT-363 | LT-603 | LT-363.N | LT-1003.N

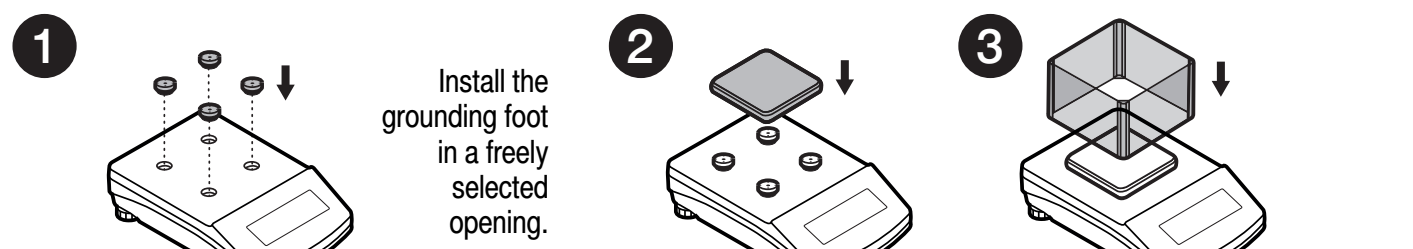

Models: LT-1202.C | LT-2102.C | LT-4502.C | LT-1202 | LT-2102 | LT-4502 | LT-2102.N | LT-4502.N

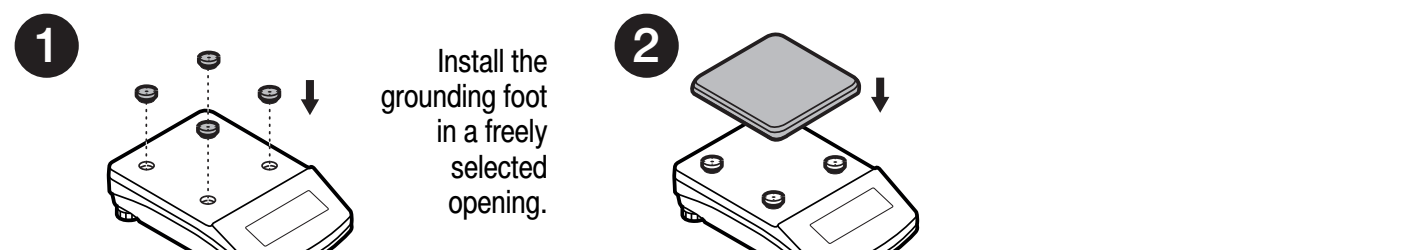


Models: LT-6002.C | LT-6002

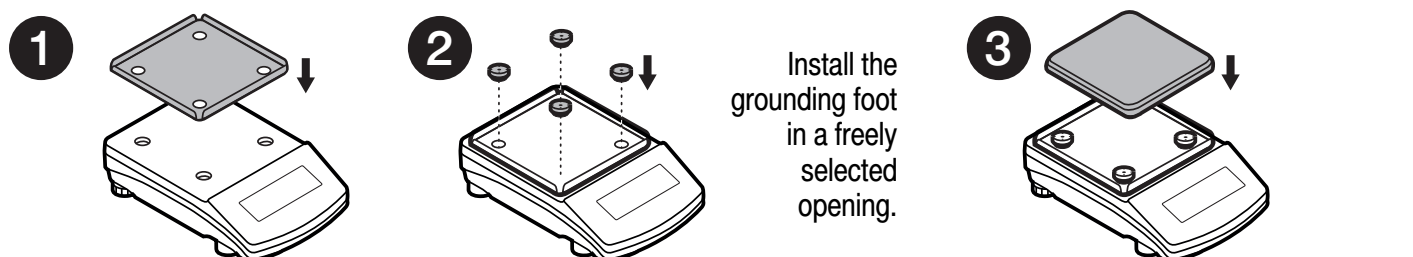


6. PREPARING FOR WORK


6.1. Balance temperature stabilization time

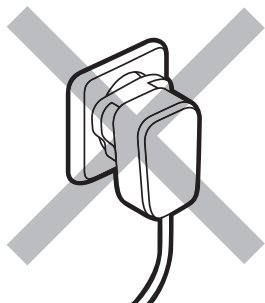


Prior to switching the device on it is necessary to ensure that it has reached a temperature equal to room temperature.

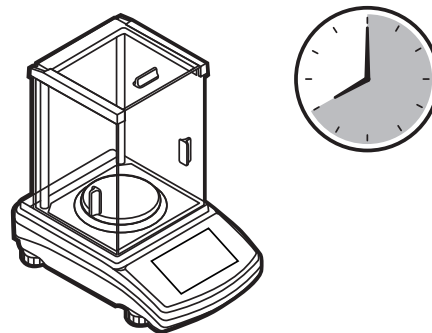



Balance temperature stabilization time ranges between 1 - 8 hours.

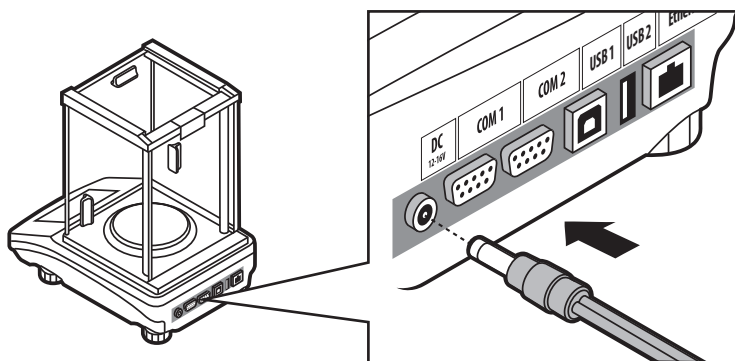

Connect the power adapter to DC connector.

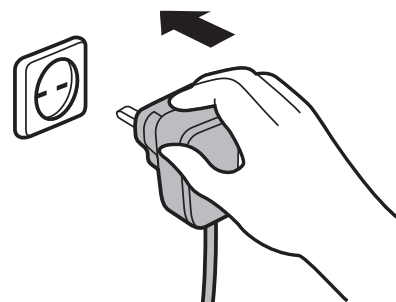


Connect the power adapter to the mains.

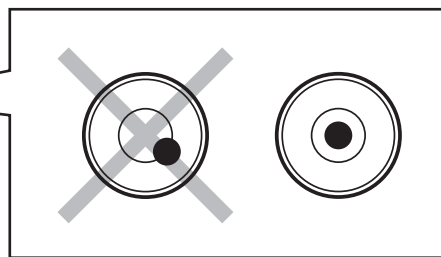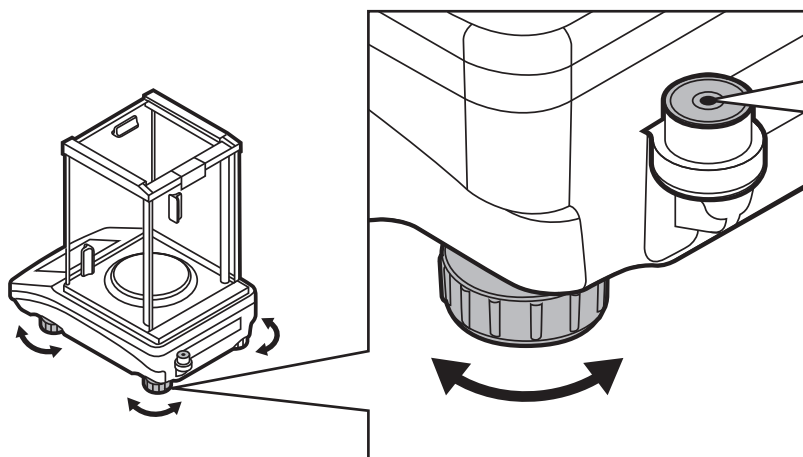


To level the balance, turn its feet and keep turning the feet until the air bubble takes the central position.

7. PANEL AND SCREEN

7.1. Panel keys


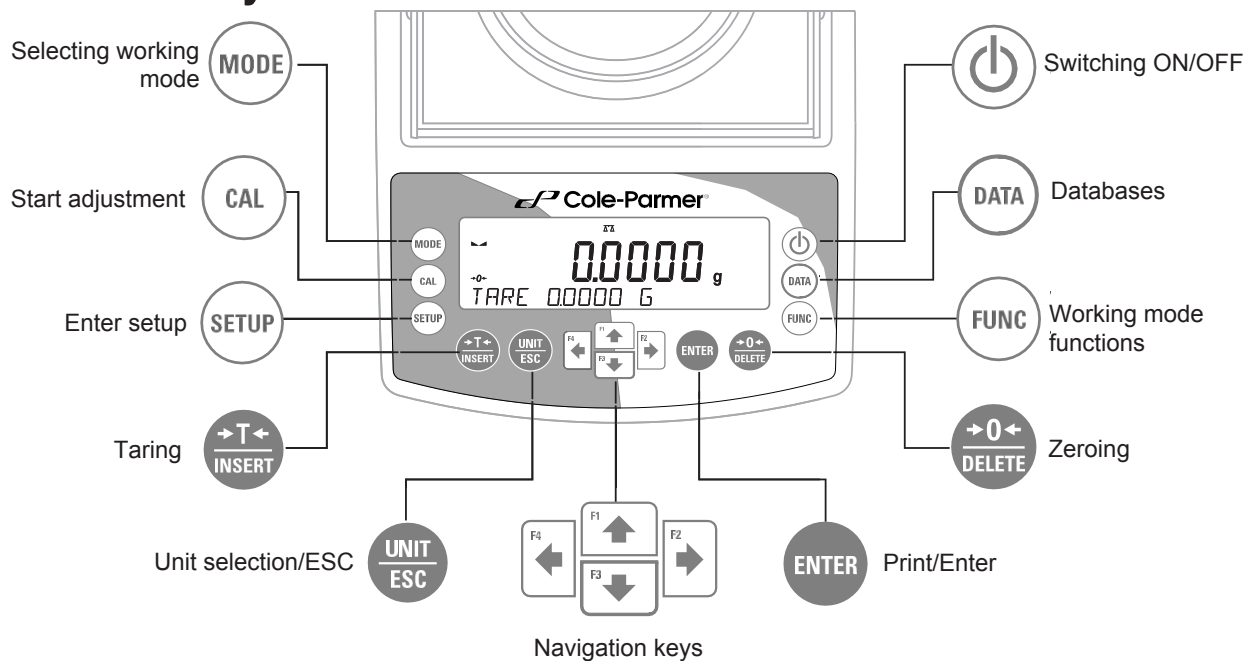


7.2. Home screen

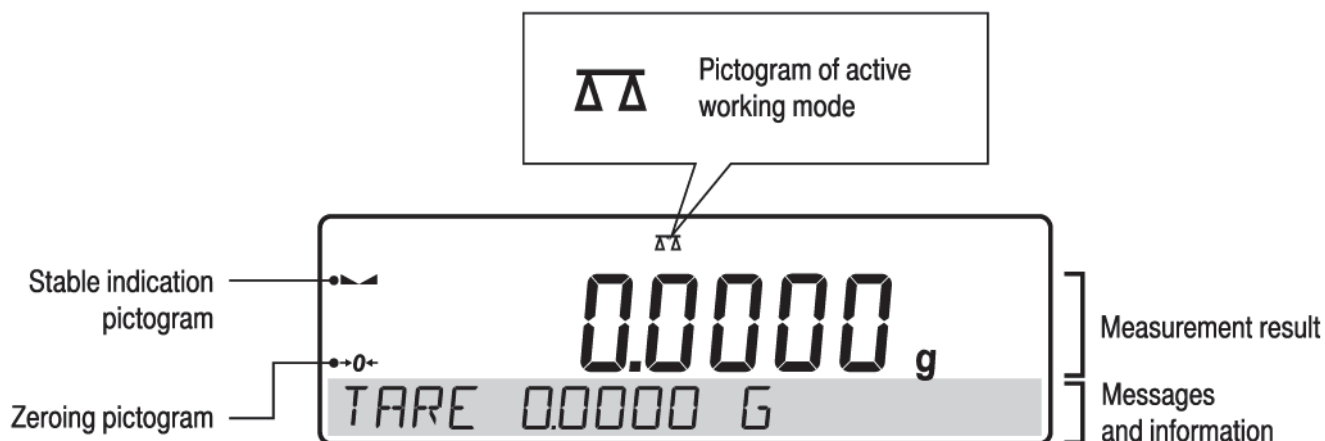

8. BASIC OPERATIONS

8.1. Adjustment-LA.C/LT.C AND LA.N/LT.N Models

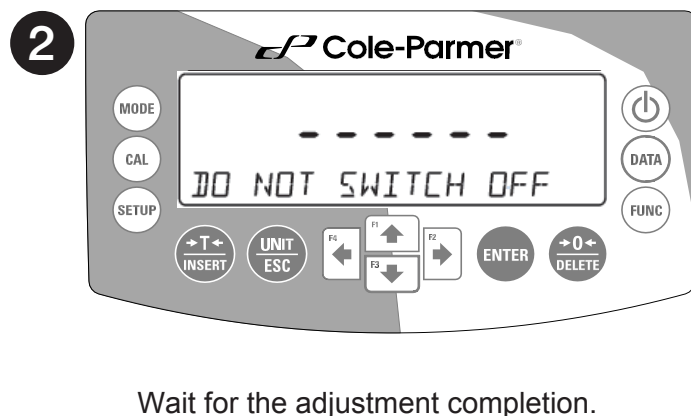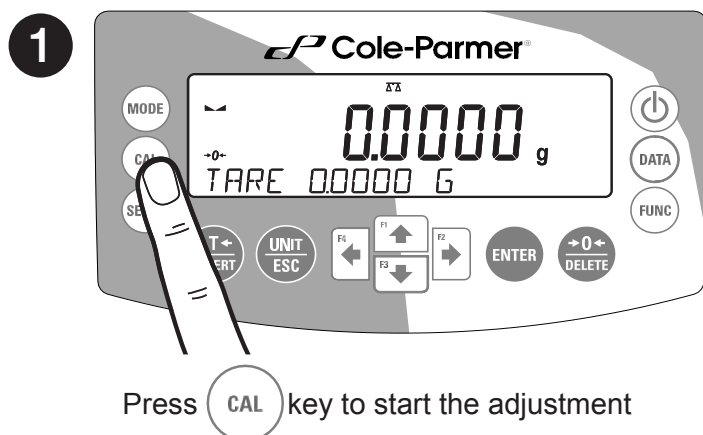

8.2. Adjustment-LA AND LT Models





External adjustment is carried out using an external mass standard of the right accuracy and weight value, which value depends on balance type and capacity.




Prior adjustment prepare the right mass standard. You are recommended to use mass standard of class F1 or F2.


View the table and select the mass standard you need.

Balance model	Mass standard [g]	Balance model	Mass standard [g]
LA-64	50	TT-1003	1 000
LA-124	100	TT-2102	1 000
LA-214	200	TT-4502	2 000
LA-314	200	TT-6002	5 000
LT-363	200	TT-6001	5 000
LT-603	500	TT-10001	10 000

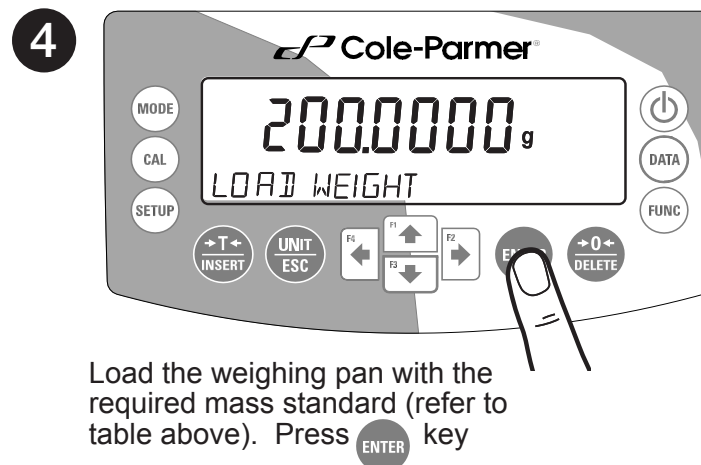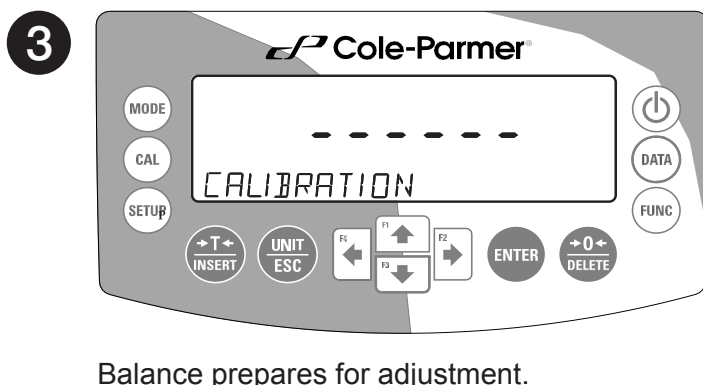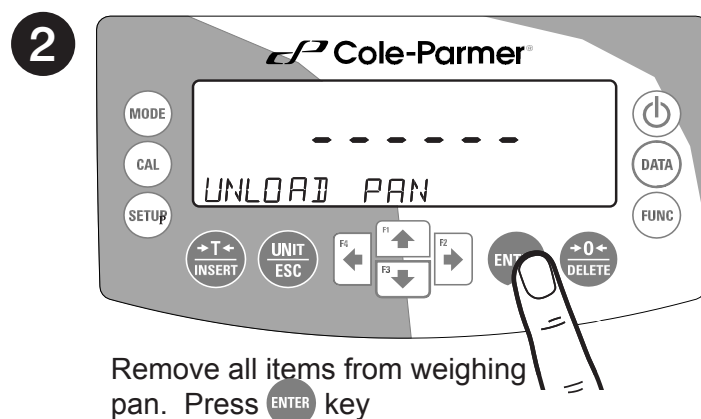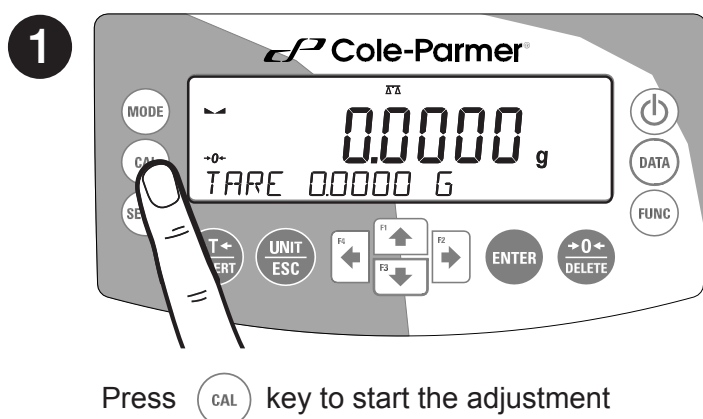

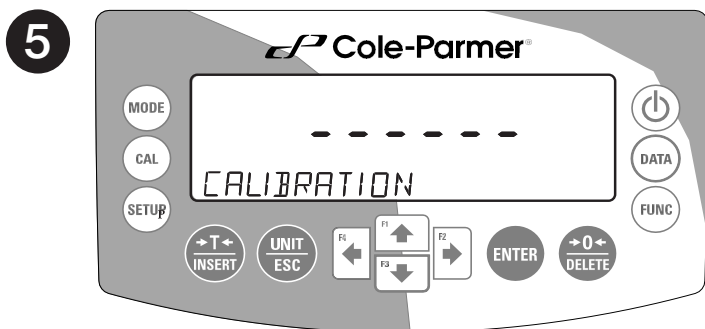


Balance completes adjustment.

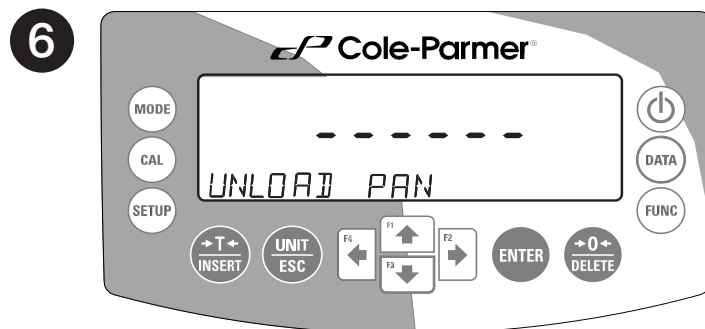


Unload the weighing pan. The balance has been calibrated.

8.3. Zeroing

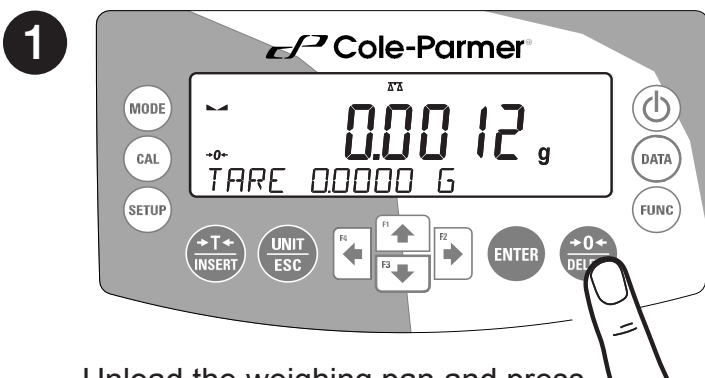


Unload the weighing pan and press "Zeroing" button.

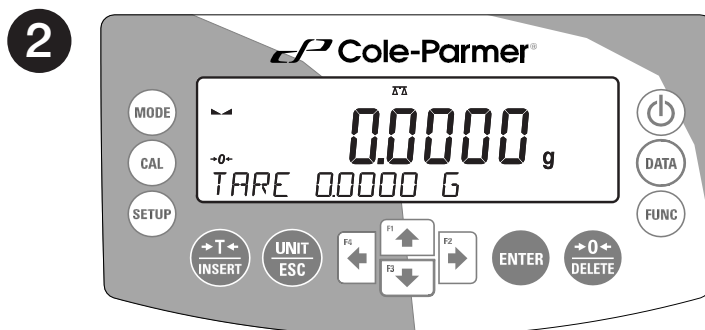


The balance has been zeroed.

8.4. Taring

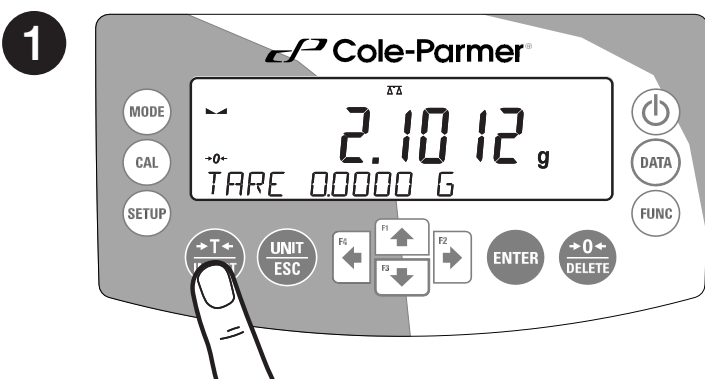


When the weighing result has been displayed press "Tare" button.

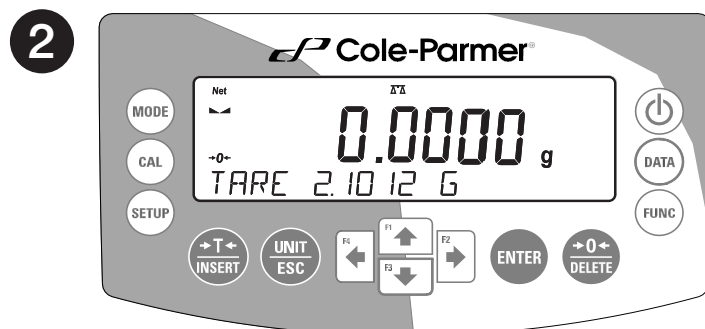




The balance has been tared.

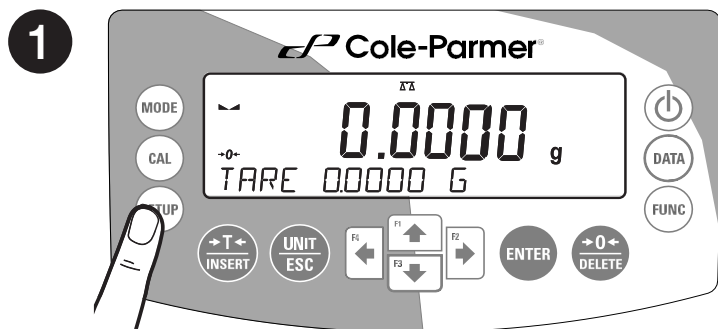
8.5. Working modes accessibility

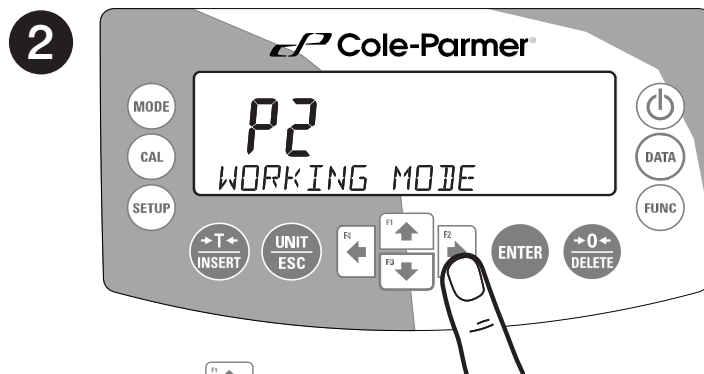


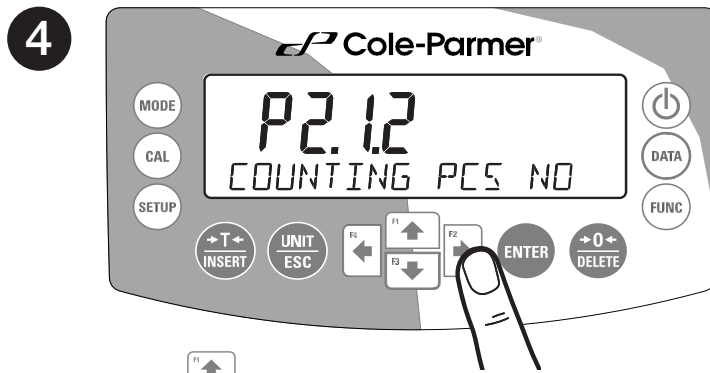
Press  to enter "Setup" menu.



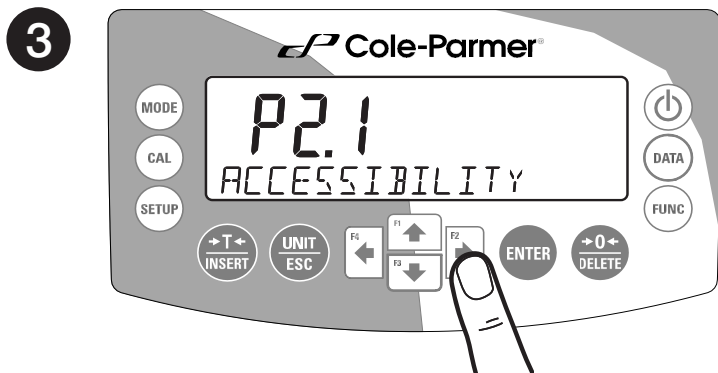


Using  keys select "Working mode" and press  key





In the "Accessibility" position, press  key

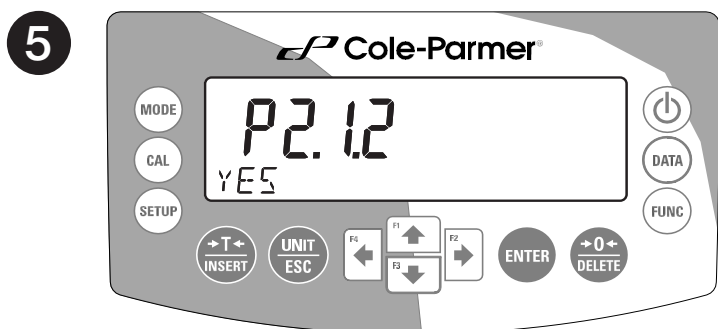

Using  keys to select working modes for which accessibility is to be set and press  key.




Using  keys to set accessibility parameter to "Yes" value for a selected working mode and press  key to confirm.




In order to enable other working modes, repeat the steps: **4** and **5**.

8.6. Selecting working mode

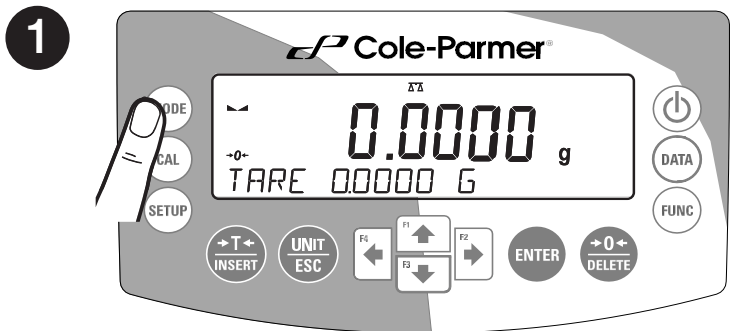

Press **MODE** key to enter working modes menu.

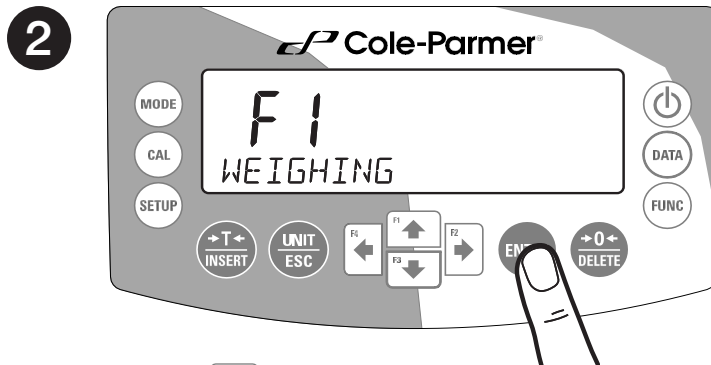

Using **F1** / **F3** keys, select working mode and press **ENTER** key to confirm.


The menu features the following working modes:

- Weighing
- Parts counting
- Checkweighing
- Dosing
- Deviations
- Density Determination of Solids
- Density Determination of Liquids
- Statistics
- Totalising
- Peak Hold
- Pipettes Calibration




Detailed overview of the settings of the working modes is to be found in balance's main user manual.




8.7. Weighing unit accessibility

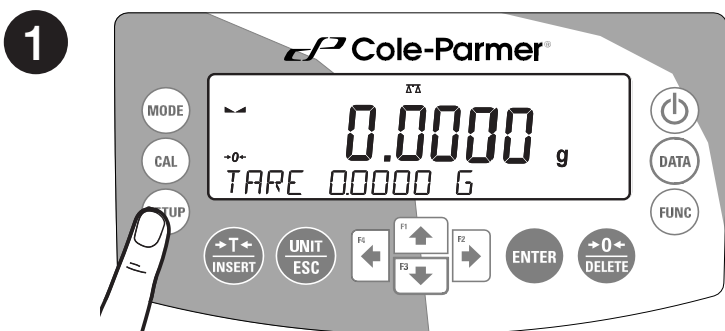

Press **SETUP** to enter "Setup" menu.

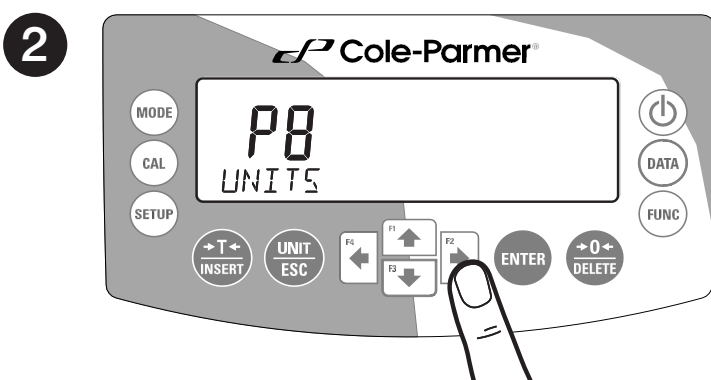


Using **F1** / **F3** keys, select "Units" and press **F2** key

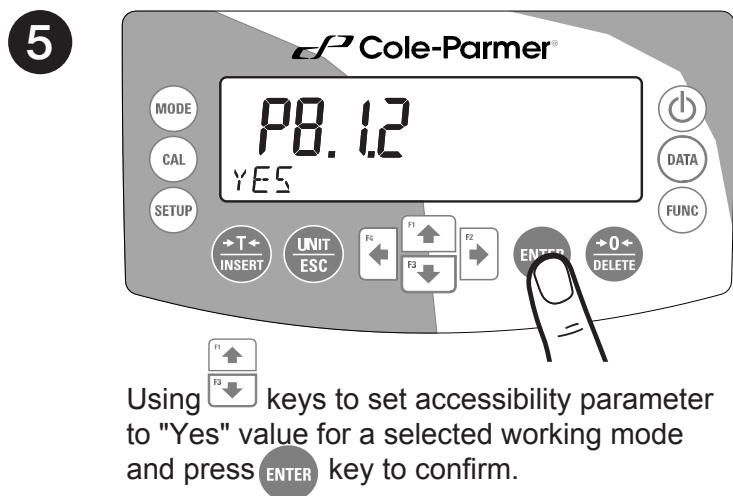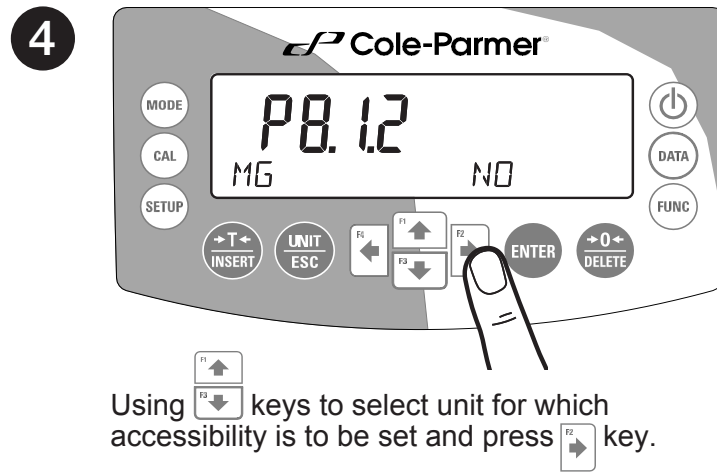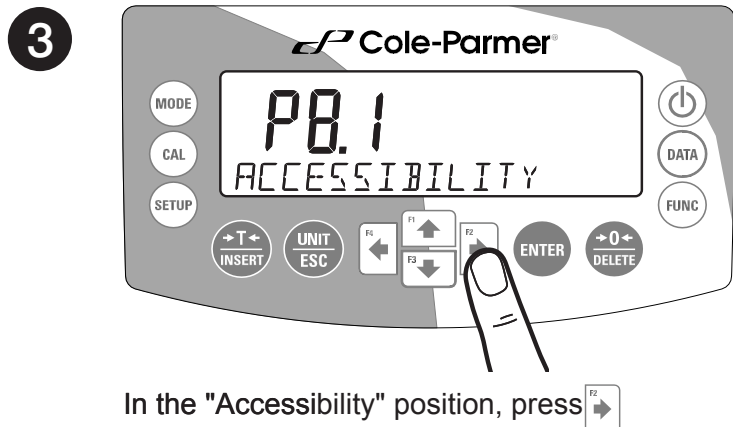

i In order to enable other working modes, repeat the steps: **4** and **5**.

8.8. Weighing unit selection

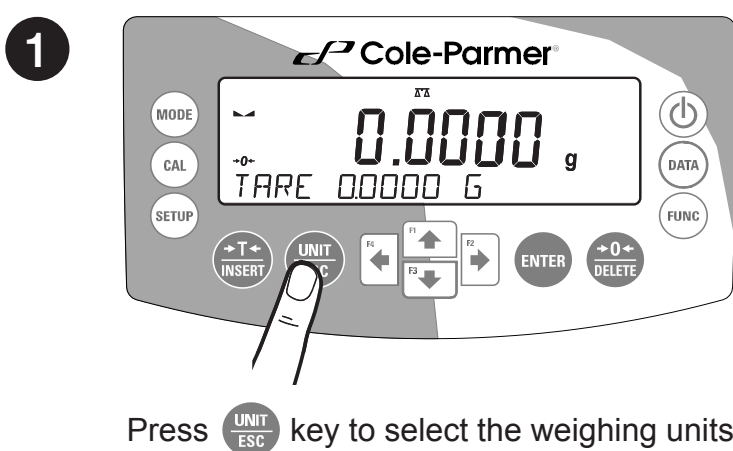

The balance enables selecting the following weighing units:

- Gram [g]*
- Miligram [mg]*
- Kilogram [kg]*
- Carat [ct]*
- Pound [lb]
- Ounce [oz]
- Troy ounce [ozt]
- Pennyweight [dwt]
- Hong Kong Tael [tlh]
- Singapore tael [tls]
- Taiwanese tael [tlt]
- Chinese tael [tlc]
- Momme [mom]
- Grain [gr]
- Tical [ti]
- Newton [N]


**Units for .N models*

9. SETTINGS




Some balance settings are accessible for Administrator exclusively.
Prior balance parameters setup, log in as the Administrator.


9.1. Administrator's login

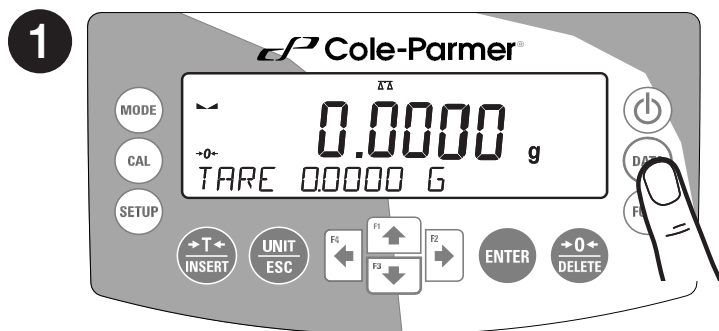


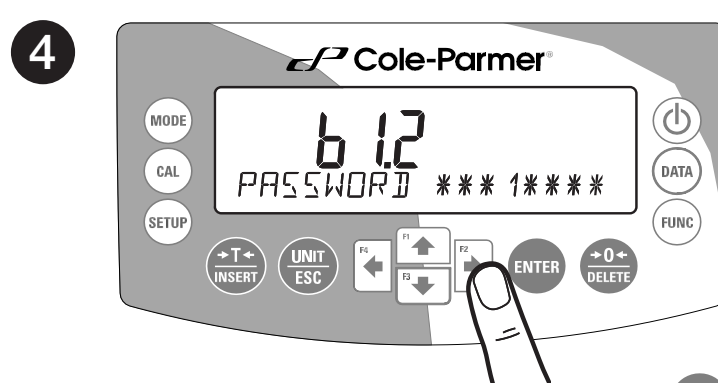
Press **DATA** key to enter "Database" menu

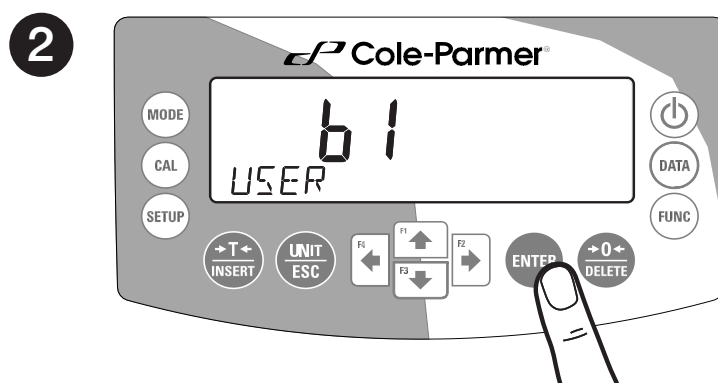


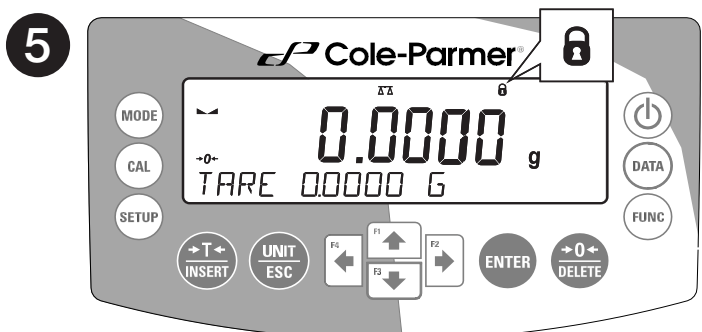
To enter user parameters, press **ENTER** key

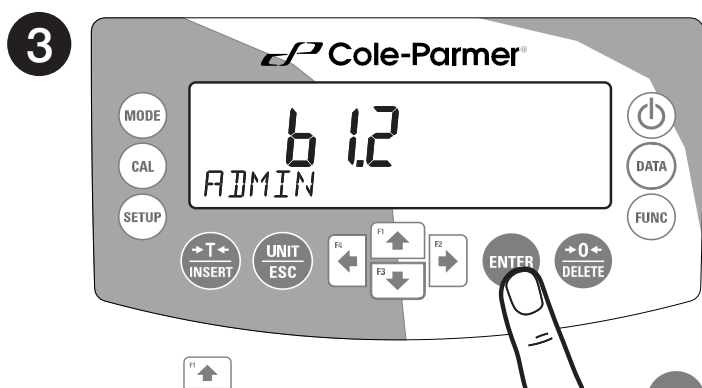

Using  keys select "Admin" and press **ENTER** key to confirm



Using  keys select "1111" and press **ENTER** key to confirm.



You have logged in as the administrator.




Upon logging in pictogram is displayed 

9.2. User settings




Prior balance users setup, log in as the Administrator.

1

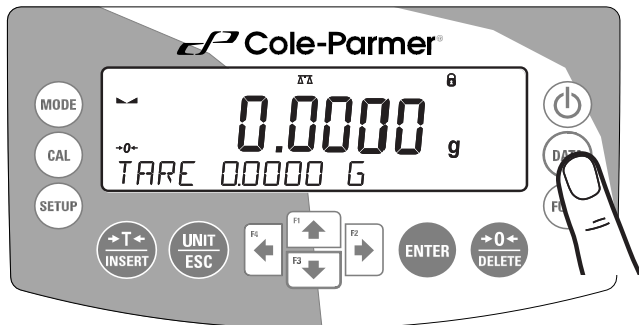


Press key to enter "Database" menu

2

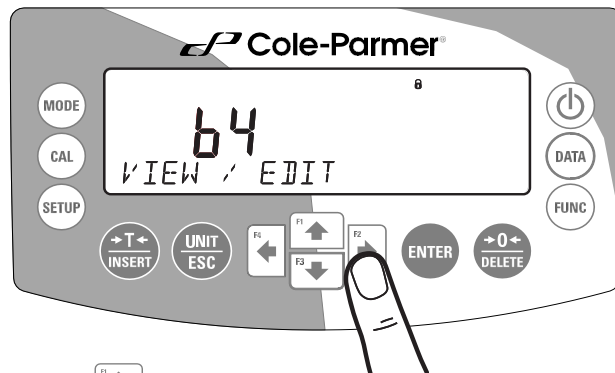


Using keys to select "View/Edit" and press key to confirm

3

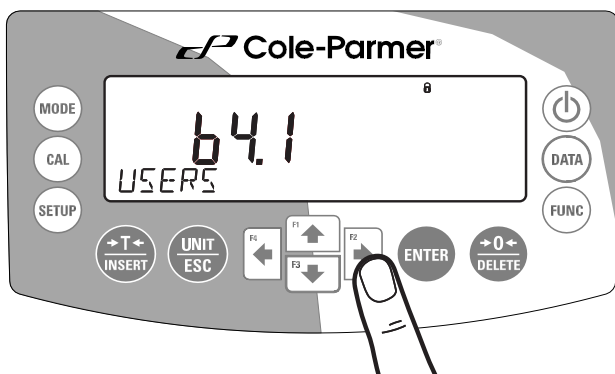


To select "Users" parameters, press key

4

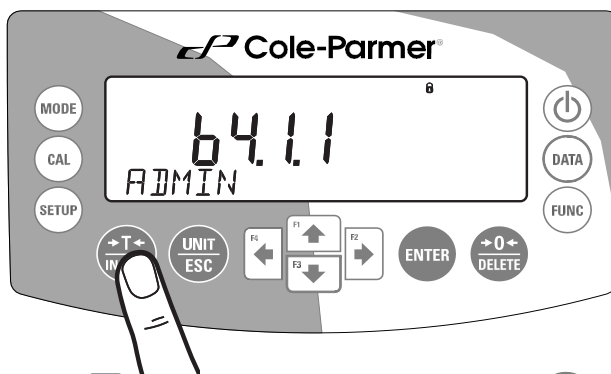

Using keys select "Admin" and press key to confirm.


5

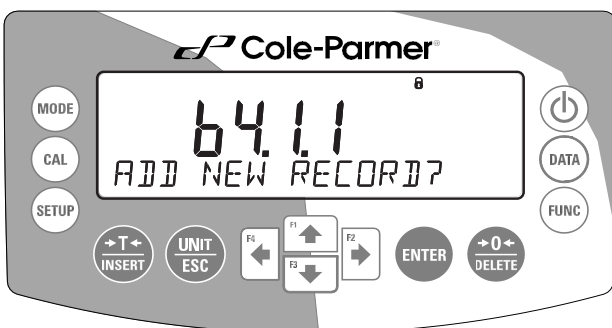


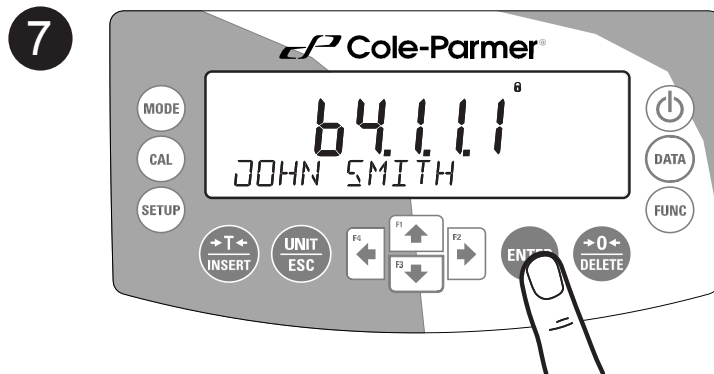
Press key to add new user.



In the following steps, set:

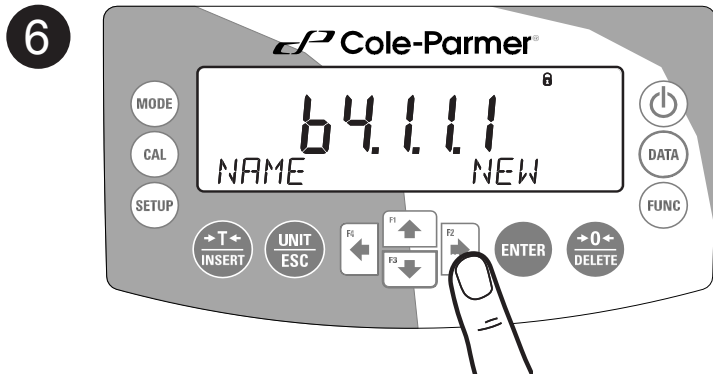
- User name
- Code
- Password
- Permissions level
- Language




Press  key to add new user.



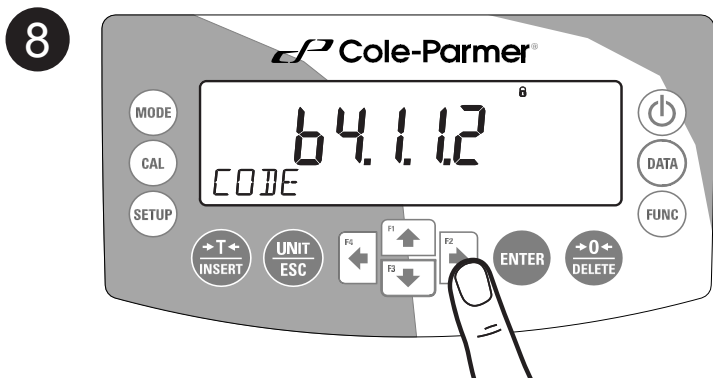


Using  keys to enter user name and press  key to confirm



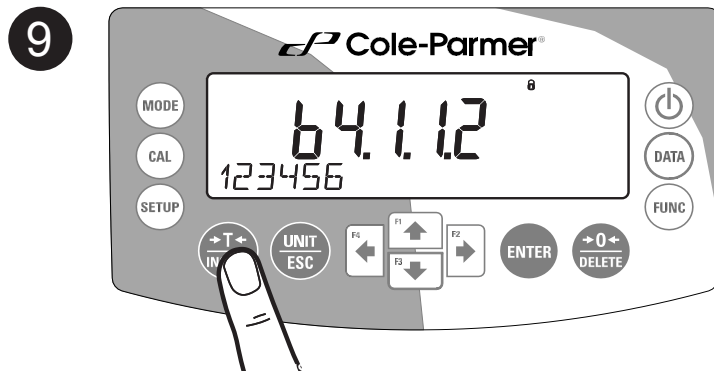


Using  keys select "Code" and press  key



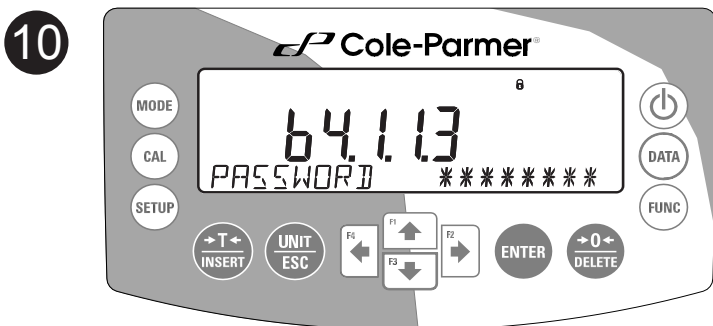

Using  keys user code and press  key to confirm




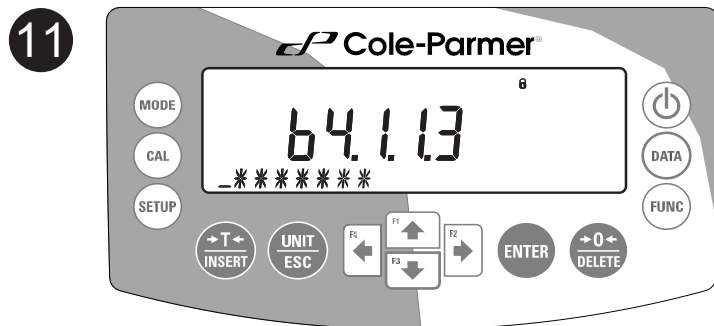

Using  keys select "Password" and press  key to confirm




Using  keys enter user password and press  key to confirm.

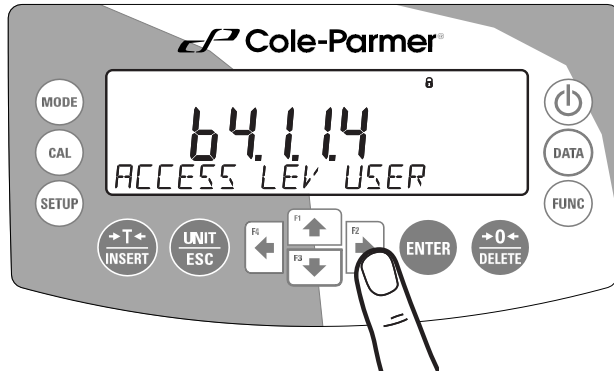

12




Using  keys select "Access Level" and press  key to confirm.

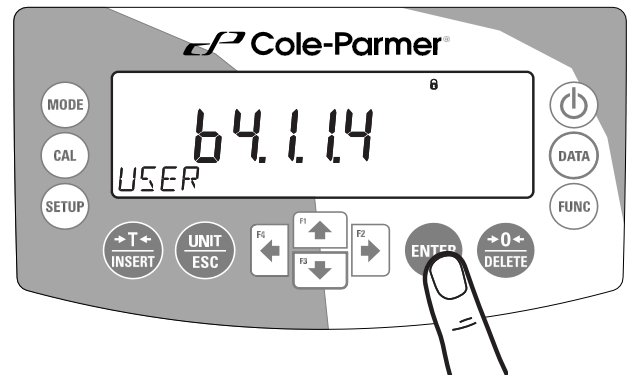

13




Using  keys select permissions level and press  key to confirm.

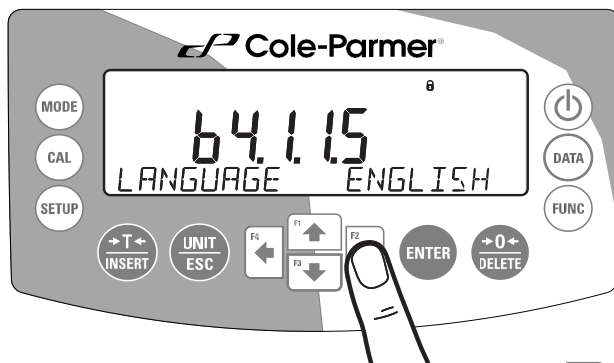

14




Using  keys select "Language" and press  key to confirm

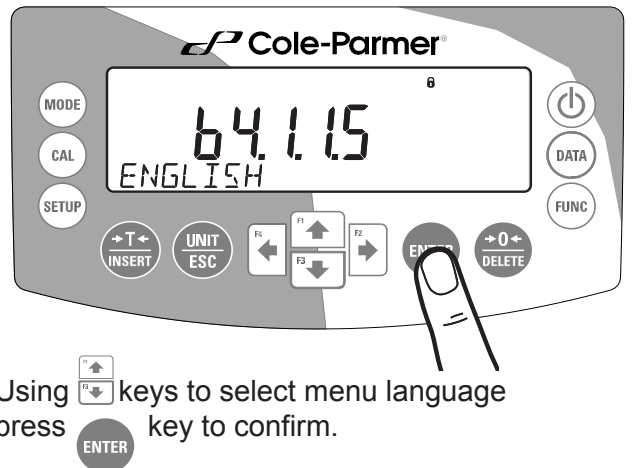15




Using  keys to select menu language press  key to confirm.

10. PERIPHERAL DEVICES CONNECTORS

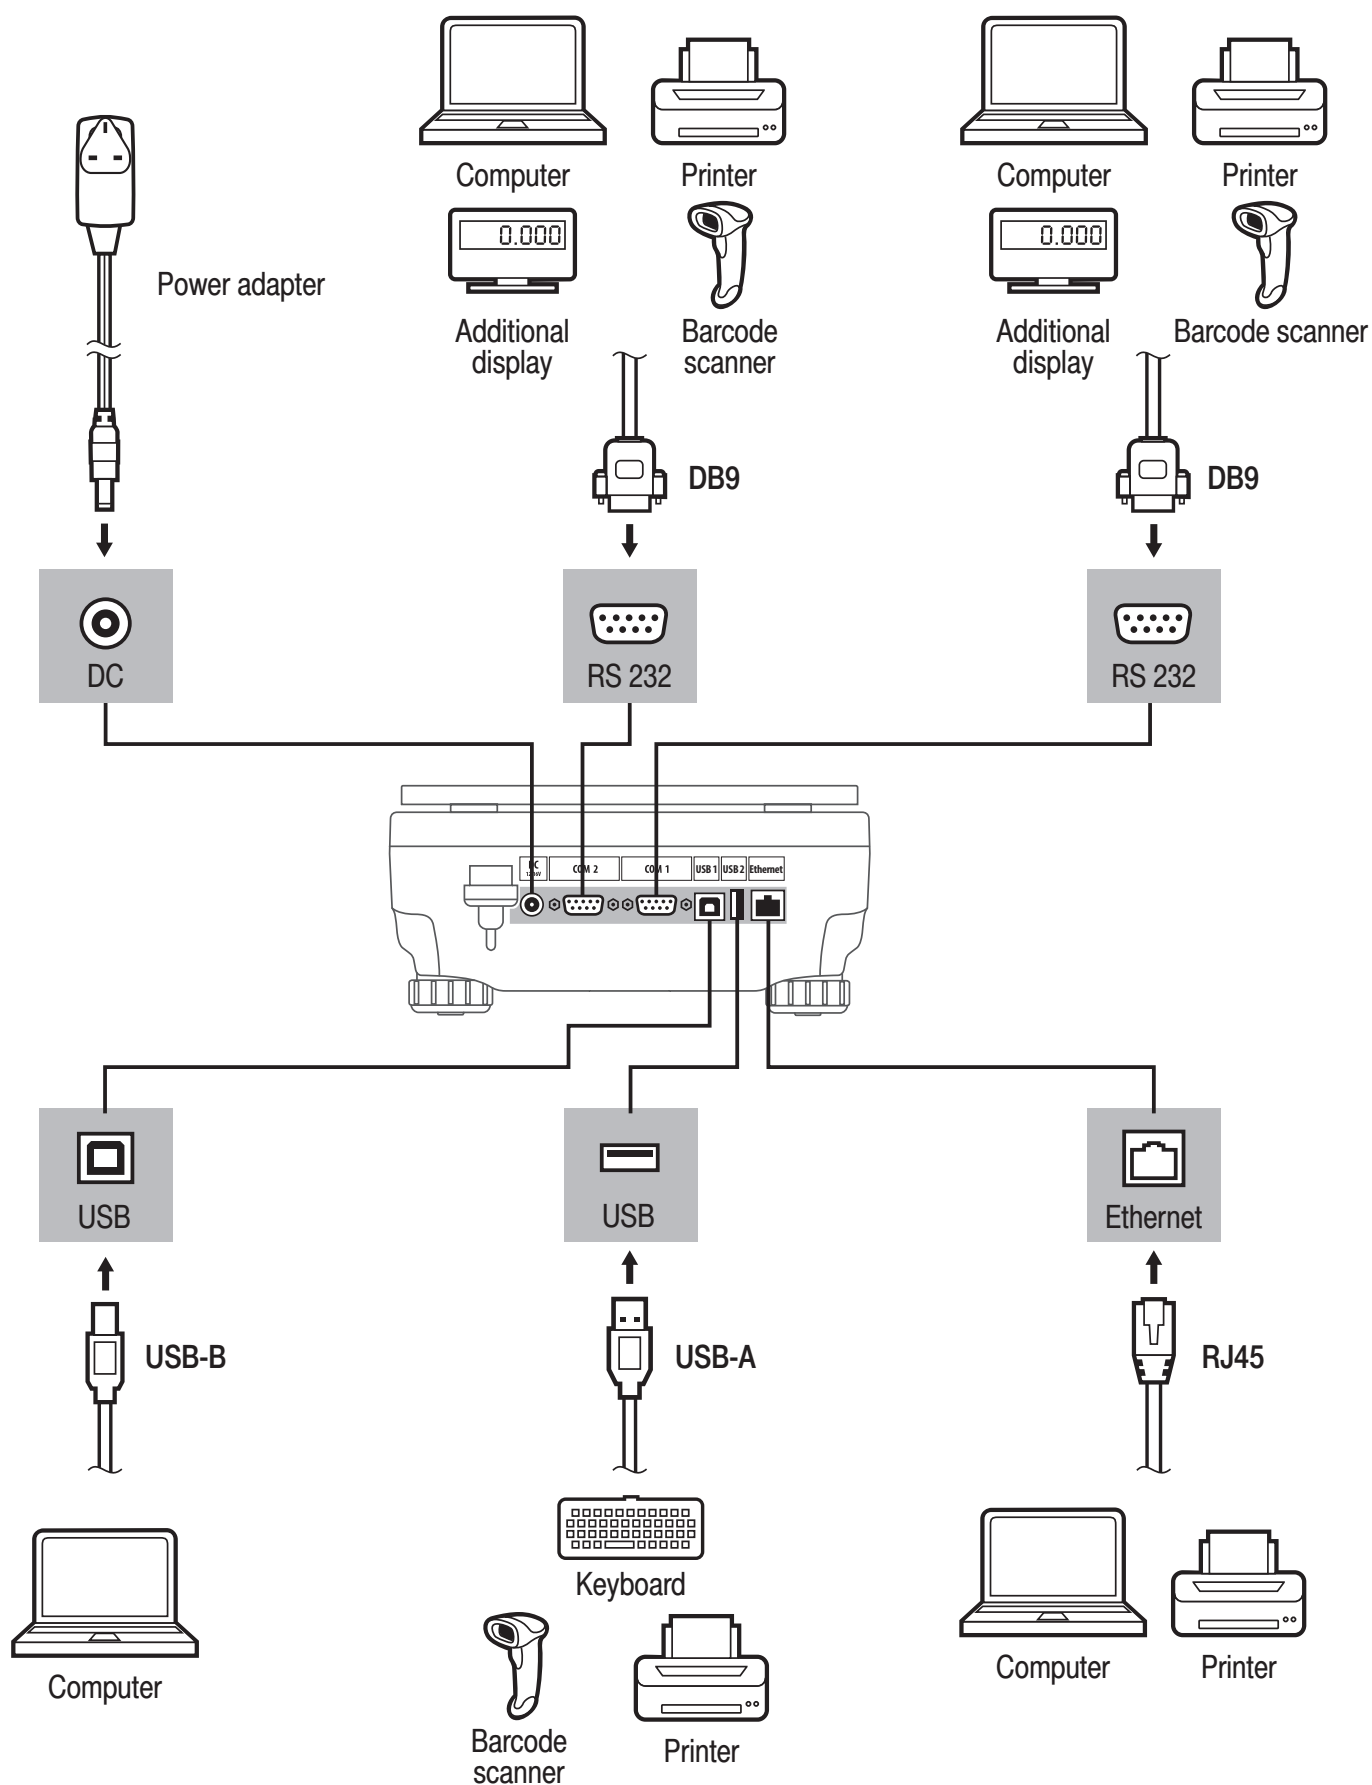


11. DEVICE CLEANING


11.1. General Recommendations

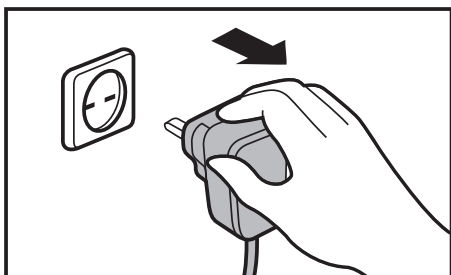

Prior to cleaning, it is necessary to disconnect the balance from the mains.

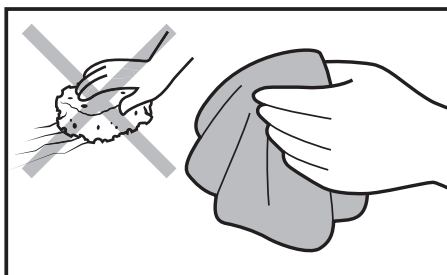

Use soft cloths made of microfiber, natural fiber or man-made fiber. Avoid using abrasive cloths or cloths that might scratch the surface.

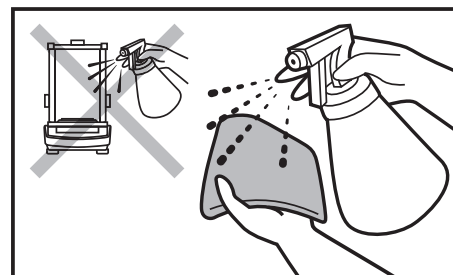

Apply the cleanser onto the cloth first. Avoid applying the cleanser directly onto the device.




Avoid using cleansers containing chlorine, corrosive chemicals and bleach. Do not use cleansers containing abrasive substances or scouring preparations.

11.2. Glass components

Prior to cleaning the glass panes, it is necessary to disassemble them first. For detailed instruction on panes disassembly, refer to user manual.


Clean glass components using a solution of water and detergent (liquid soap, dish-washing detergent, glass cleaner, etc.). In case of heavy contamination, a mild solution of vinegar or baking soda can be used.

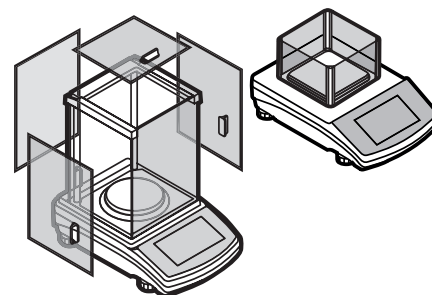

11.3. Plastic components

Prior to cleaning the plastic housing, it is necessary to disassemble weighing pan components (cover, weighing pan, etc.).


Clean plastic components using a solution of water and detergent (liquid soap, dish-washing detergent, glass cleaner, etc.).

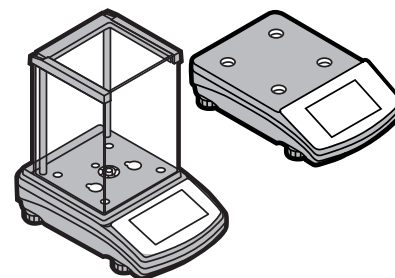

11.4. Stainless steel components

Prior to cleaning the stainless steel components, it is necessary to disassemble them first.

Clean stainless steel components using a solution of water and detergent (liquid soap, dish-washing detergent, glass cleaner, etc.). In case of heavy contamination, a mild solution of vinegar or baking soda can be used.

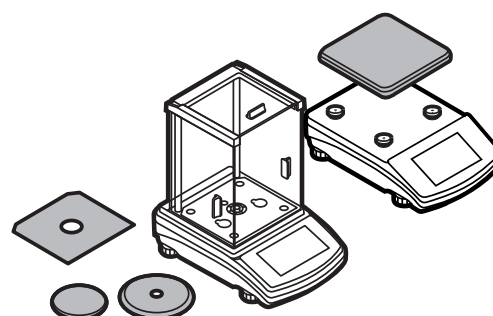



625 East Bunker Court Vernon Hills
IL 60061 USA

Phone: 1-800-323-4340

Fax: 1-847-247-2929

E-Mail: sales@coleparmer.com